

APOGEE QUANTUM SENSORS

Original X & Full-spectrum Series



The photosynthetically active radiation measurement tool of choice for lighting researchers

Features

Apogee Instruments Quantum Sensors are the tool of choice for researchers and agricultural professionals measuring photosynthetically active radiation (PAR) all over the world. Apogee offers two types of quantum sensors: a Full-spectrum Quantum and Original X Quantum Sensor. Consult our spectral response graph to decide which model is right for your application.

Accurate, Stable Measurements

Cost-effective, original quantum sensors work well for broadband radiation sources (sun, high-pressure sodium, metal halide, cool white fluorescent lamps), while full-spectrum sensors are good for all light sources, including LEDs. Offers a self-cleaning, cosine-corrected head that is fully-potted for a waterproof design.


Typical PPFD Measurement Applications

- Incoming and reflected PPFD over and under plant canopies in greenhouses, in fields, and in growth chambers
- Aquatic environments including salt water aquariums and freshwater lakes and streams

Calibration Traceability

Apogee SQ series quantum sensors are calibrated through side-by-side comparison to the mean of four transfer standard sensors under a reference lamp. The reference sensors are recalibrated with a quartz halogen lamp traceable to the National Institute of Standards and Technology (NIST).

Spectral Response

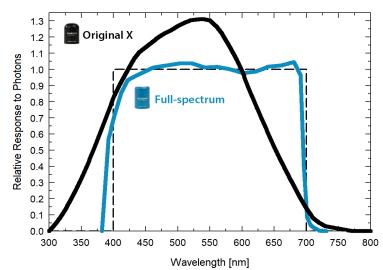

Spectral response of **original X quantum sensor (black)** and **fullspectrum quantum sensor (blue)** compared to defined response of plants to radiation (dashed).

Spectral Errors

| | Apogee SQ-500 | Apogee SQ-100X | LI-COR LI-190 | Kipp & Zonen PQS 1 |
|---|------------------|-------------------|------------------|--------------------------|
| Sun (Clear Sky) | 0.0 | 0.0 | -0.4 | -1.0 |
| Sun (Cloudy Sky) | 0.1 | 0.2 | -0.2 | -1.3 |
| Sun (Reflected from Grass Canopy) | -0.3 | 5.0 | -0.8 | 1.1 |
| Sun (Transmitted below Wheat Canopy) | 0.1 | 7.0 | -0.1 | -0.3 |
| Cool White Fluorescent (T5) | 0.0 | 7.2 | 0.0 | 0.0 |
| Metal Halide | 0.9 | 6.9 | 0.2 | -1.7 |
| Ceramic Metal Halide | 0.3 | -8.8 | 0.4 | -0.7 |
| High Pressure Sodium | 0.1 | 3.3 | 1.3 | 1.4 |
| Red LED (667 nm peak, 20 nm full-width half-maximum) | 2.8 | -56.7 | 3.5 | -1.8 |
| Red, Blue, White LED Mixture (60 % Red, 25 % White, 15 % Blue) | -2.0 | -21.2 | 2.6 | -1.7 |



FULL-SPECTRUM QUANTUM SENSORS

All othe

models

-500 Q-520

apøgee

SQ-500 Series

Provides research-grade measurements under all light sources, including LEDs

Output Options

- 0 to 40 mV
- 0 to 5 V
- USB
- Modbus
- 4 to 20 mA
 SDI-12
- or hand-held meter

• 0 to 2.5 V

• or hand-held met



apøgee

Product Specifications

| | SQ-500-SS | SQ-512-SS | SQ-514-SS | SQ-515-SS | SQ-520 | SQ-521-SS | SQ-522-SS | |
|--|---|--|--|---|--|--|--|--|
| Power Supply | Self-powered | 5 to 24 V DC | 12 to 24 V DC | 5.5 to 24 V DC | 5 V USB power source | 5.5 to 24 V DC | | |
| Current Draw | - | At 12 V is 57 μΑ | maximum of 20 mA | At 12 V is 57 μA | 61 mA when logging | 1.4 mA (quiescent), 1.8 mA (active) | RS-232 37 mA; RS-485 quiescent 37 mA, active 42 mA | |
| Output (sensitivity) | 0.01 mV per μmol m ⁻² s ⁻¹ | 0.625 mV per μmol m ⁻² s ⁻¹ | 0.004 mA per μmol m ⁻² s ⁻¹ | 1.25 mV per μmol m ⁻² s ⁻¹ | _ | | | |
| Resolution | | _ | | | 0.1 μmol m ⁻² s ⁻¹ – | | | |
| Calibration Factor (reciprocal of output) | 100 μmol m ⁻² s ⁻¹ per mV | 1.6 μmol m ⁻² s ⁻¹ per mV | $\begin{array}{c} 250 \ \mu mol \ m^{-2} \ s^{-1} \\ per \ mA \end{array}$ | 0.8 μmol m ⁻² s ⁻¹ per mV | Custom for each sensor and stored in the firmware | | | |
| Calibration Uncertainty | ± 5 % | | | | | | | |
| Output Range | 0 to 40 mV | 0 to 2.5 V | 4 to 20 mA | 0 to 5 V | USB | SDI-12 | Modbus | |
| Measurement Repeatability | Less than 0.5 % | | | | | | | |
| Long-term Drift | Less than 2 % per year | | | | | | | |
| Non-linearity | Less than 1 % (up to 4000 μ mol m ⁻² s ⁻¹) | | | | | | | |
| Response Time | Less than 1 ms | | | Software updates every second | Less than 0.6 s | Less than 200 ms | | |
| Field of View | 180° | | | | | | | |
| Spectral Range | 389 to 692 nm \pm 5 nm (wavelengths where response is greater than 50 %) | | | | | | | |
| Directional (cosine) Response | ± 5 % at 75° zenith angle | | | | | | | |
| Temperature Response | -0.11 ± 0.04 % per C | | | | | | | |
| Operating Environment | -40 to 70 C; 0 to 100 % relative humidity; can be submerged in water up to depths of 30 m | | | | | | | |
| Dimensions | 24 mm diameter, 37 mm height | 30.5 m | ım diameter, 37 mn | n height | 24 mm diameter,30.5 mm diameter,37 mm height37 mm height | | | |
| Mass (5 m of cable) | 100 g | 100 g 140 g | | | 100 g | 140 g | | |
| Warranty | 4 years against defects in materials and workmanship | | | | | | | |



ORIGINAL X QUANTUM SENSORS

SQ-100X, SQ-200X, & SQ-400X Series



Measure photosynthetically active radiation (PAR) in µmol m⁻² s⁻¹

Output Options

• 0 to 400 mV


SQ-100X


- 0 to 5 V
- USB
- Modbus
- 0 to 2.5 V • 4 to 20 mA • SDI-12
- or hand-held meter



Product Specifications

| | SQ-100X-SS | SQ-202X-SS | SQ-204X-SS | SQ-205X-SS | SQ-420X | SQ-421X-SS | SQ-422X-SS |
|---|---|---|--|--|--|--|--|
| Power Supply | Self-powered | 5 to 24 V DC | 7 to 24 V DC | 5.5 to 24 V DC | 5 V USB power source | 5.5 to 24 V DC | |
| Current Draw | - | 10 μΑ | 22 mA maximum; 2 mA quiescent | 10 µA | 61 mA when logging | 1.4 mA (quiescent), 1.8 mA (active) | RS-232 37 mA; RS-485 quiescent 37 mA, active 42 mA |
| Output (sensitivity) | 0.1 mV per µmol m ⁻² s ⁻¹ | 1 mV per μmol m ⁻² s ⁻¹ | 0.004 mA per μ mol m ⁻² s ⁻¹ | 2 mV per µmol m⁻² s⁻¹ | _ | | |
| Calibration Factor (reciprocal of output) | 10 µmol m⁻² s⁻¹ per mV | 1 μmol m ⁻² s ⁻¹ per mV | 250 μmol m ⁻² s ⁻¹ per mA | 0.5 µmol m ⁻² s ⁻¹ per mV | Custom for each sensor and stored in the firmware | | |
| Calibration for Uncertainty | ± 5 % | | | | | | |
| Output Range | 0 to 250 mV | 0 to 2.5 V | 4 to 20 mA | 0 to 5 V | USB | SDI-12 | Modbus |
| Measurement Repeatability | Less than 0.5 % | | | | | | |
| Long-term Drift | Less than 2 % per year | | | | | | |
| Non-linearity | Less than 1 % (up to 2500 μ mol m ⁻² s ⁻¹) | | | | | | |
| Response Time | Less than 1 ms | | | Software updates every second | Less than 0.6 s | Less than 200 ms | |
| Field of View | 180° | | | | | | |
| Spectral Range | 370 to 650 nm (wavelengths where response is greater than 50 % maximum) | | | | | | |
| Directional (cosine) Response | ± 5 % at 75° zenith angle | | | | | | |
| Temperature Response | -0.04 % per C | | | | | | |
| Operating Environment | -10 to 60 C; 0 to 100 % relative humidity; can be submerged in water up to 30 m | | | | | | |
| Dimensions | 24 mm diameter, 33 mm height | 30.5 mm diameter, 37 mm height24 mm diameter, 33 mm height30.5 mm diameter | | ter, 37 mm height | | | |
| Mass (5 m of cable) | 90 g | 140 g | | | 90 g | 140 g | |
| Warranty | 4 years against defects in materials and workmanship | | | | | | |

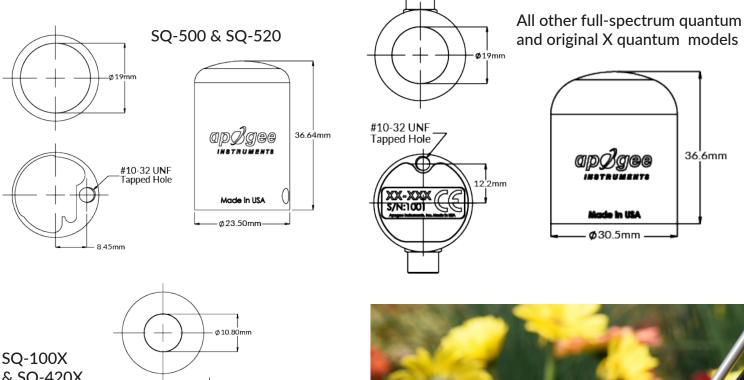

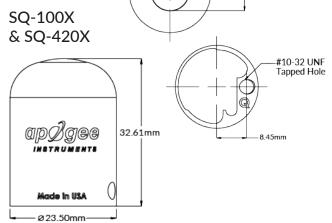



Case Study

The **Kuwait Institute for Scientific Research** used Apogee's **MQ-510** underwater full-spectrum quantum meters to help model algal species and their growth rate in Kuwait Bay. This research advances the researchers' understanding of the frequent algal bloom and fish kill incidents that typically occur in the summer.



